


This procedure explains how to add an internal standard to the digestion vessel on the ANKOM<sup>FLEX</sup> Analyte Extractor.


1. **Unscrew the red cap on the digestion vessel port that you would like to add the internal standard too.**



2. **Using a pipette, add the internal standard into the digestion vessel through the vessel port.**



3. **Screw the red cap onto the vessel port. Tighten but do not over tighten.**

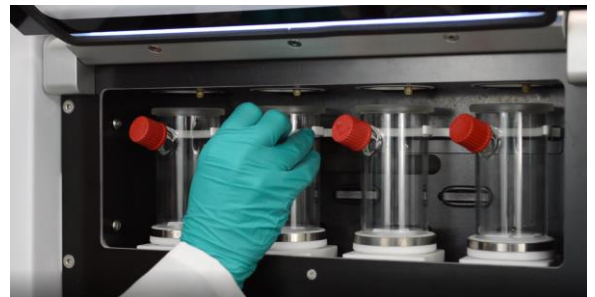

4. **Repeat for each vessel you wish to insert the internal standard.**